

CALIBRATION OF RADIOCARBON AGE TO CALENDAR YEARS

(Variables: C13/C12=-26.4:lab. mult=1)

Laboratory number: **Beta-163245**


Conventional radiocarbon age: **5850±40 BP**

2 Sigma calibrated result: **Cal BC 4790 to 4600 (Cal BP 6740 to 6560)**
(95% probability)

Intercept data

Intercept of radiocarbon age
with calibration curve: **Cal BC 4710 (Cal BP 6660)**

1 Sigma calibrated result: **Cal BC 4740 to 4690 (Cal BP 6690 to 6640)**
(68% probability)

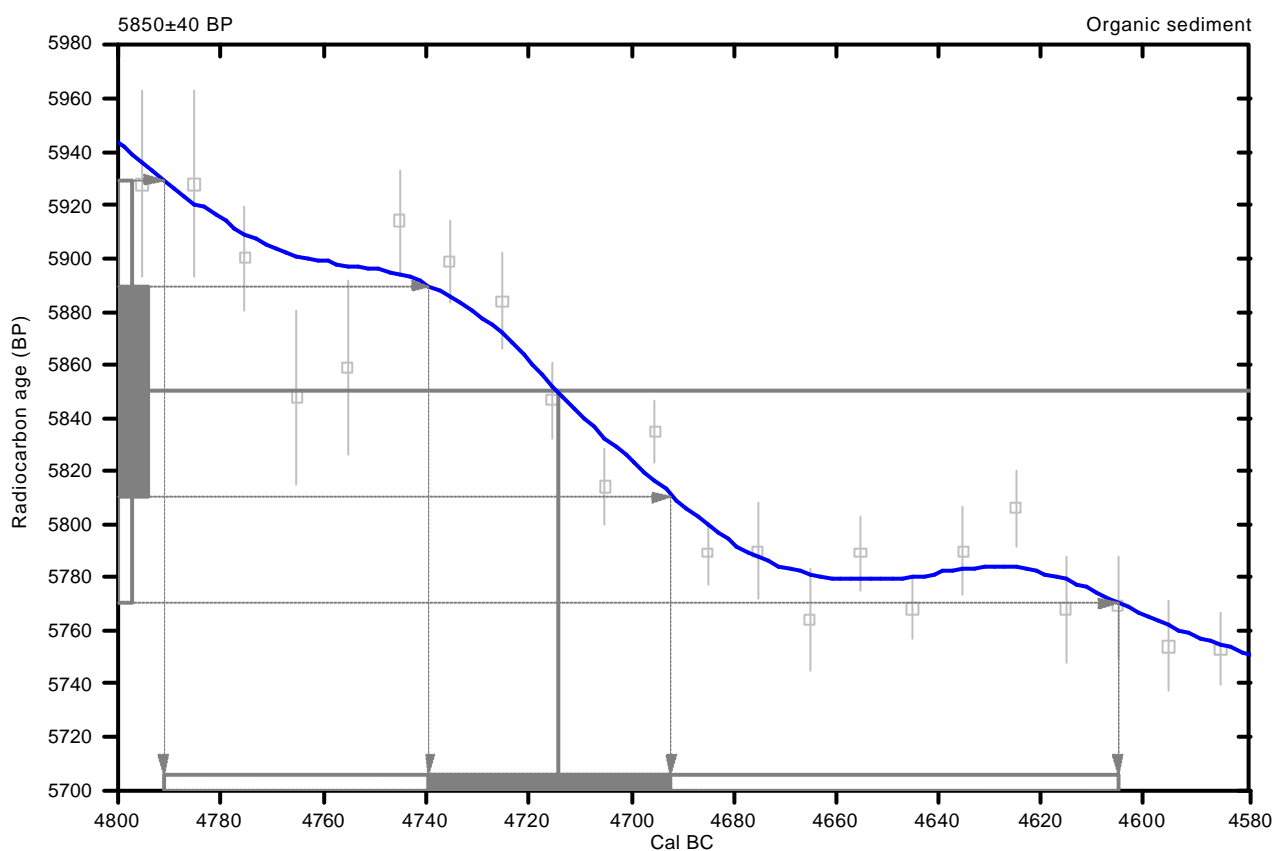

References:

Database used

Calibration Database
Editorial Comment

Stuiver, M., van der Plicht, H., 1998, Radiocarbon 40(3), pxii-xiii

INTCAL98 Radiocarbon Age Calibration

Stuiver, M., et. al., 1998, Radiocarbon 40(3), p1041-1083

Mathematics

A Simplified Approach to Calibrating C14 Dates

Talma, A. S., Vogel, J. C., 1993, Radiocarbon 35(2), p317-322

Beta Analytic Inc.

4985 SW 74 Court, Miami, Florida 33155 USA • Tel: (305) 667 5167 • Fax: (305) 663 0964 • E-Mail: beta@radiocarbon.com

CALIBRATION OF RADIOCARBON AGE TO CALENDAR YEARS

(Variables: C13/C12=-27;lab. mult=1)

Laboratory number: **Beta-163251**


Conventional radiocarbon age: **6310±40 BP**

2 Sigma calibrated result: **Cal BC 5350 to 5230 (Cal BP 7300 to 7180)**
(95% probability)

Intercept data

Intercept of radiocarbon age
with calibration curve: **Cal BC 5300 (Cal BP 7250)**

1 Sigma calibrated result: **Cal BC 5320 to 5280 (Cal BP 7270 to 7230)**
(68% probability)

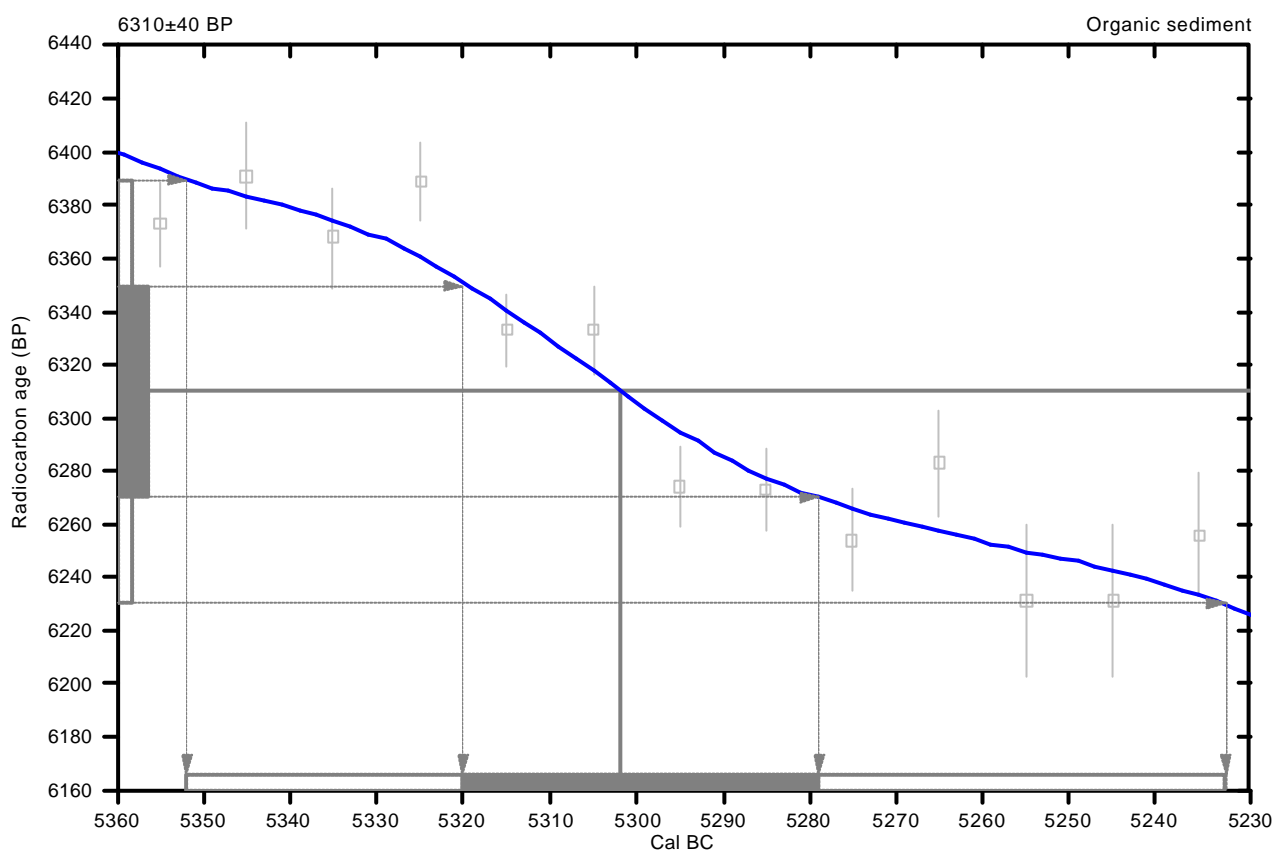

References:

Database used

Calibration Database
Editorial Comment

Stuiver, M., van der Plicht, H., 1998, Radiocarbon 40(3), pxii-xiii

INTCAL98 Radiocarbon Age Calibration

Stuiver, M., et. al., 1998, Radiocarbon 40(3), p1041-1083

Mathematics

A Simplified Approach to Calibrating C14 Dates

Talma, A. S., Vogel, J. C., 1993, Radiocarbon 35(2), p317-322

Beta Analytic Inc.

4985 SW 74 Court, Miami, Florida 33155 USA • Tel: (305) 667 5167 • Fax: (305) 663 0964 • E-Mail: beta@radiocarbon.com

CALIBRATION OF RADIOCARBON AGE TO CALENDAR YEARS

(Variables: C13/C12=-24.6:lab. mult=1)

Laboratory number: **Beta-163253**


Conventional radiocarbon age: **2870±40 BP**

2 Sigma calibrated result: **Cal BC 1140 to 920 (Cal BP 3090 to 2870)**
(95% probability)

Intercept data

Intercept of radiocarbon age
with calibration curve: **Cal BC 1020 (Cal BP 2970)**

1 Sigma calibrated result: **Cal BC 1100 to 990 (Cal BP 3050 to 2940)**
(68% probability)

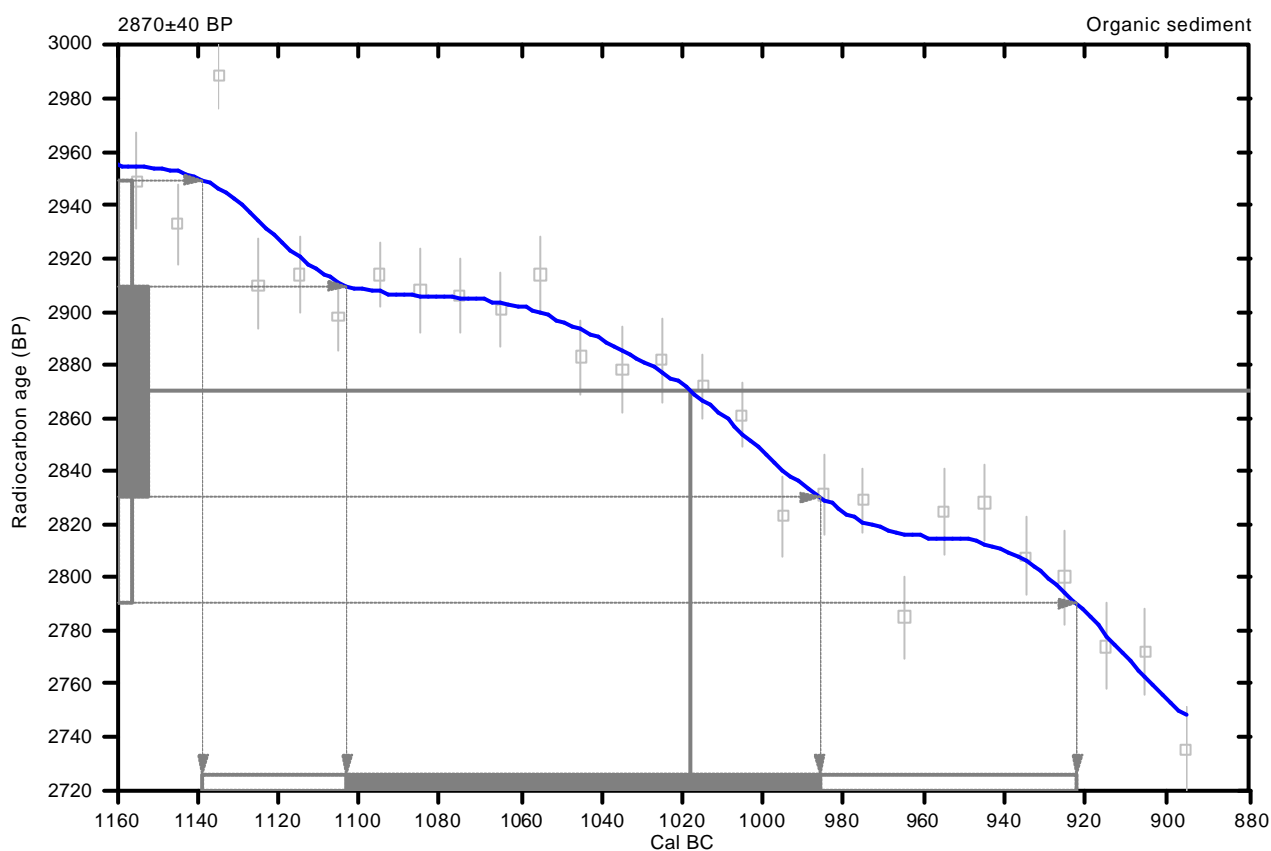

References:

Database used

Calibration Database

Editorial Comment

Stuiver, M., van der Plicht, H., 1998, Radiocarbon 40(3), pxii-xiii

INTCAL98 Radiocarbon Age Calibration

Stuiver, M., et. al., 1998, Radiocarbon 40(3), p1041-1083

Mathematics

A Simplified Approach to Calibrating C14 Dates

Talma, A. S., Vogel, J. C., 1993, Radiocarbon 35(2), p317-322

Beta Analytic Inc.

4985 SW 74 Court, Miami, Florida 33155 USA • Tel: (305) 667 5167 • Fax: (305) 663 0964 • E-Mail: beta@radiocarbon.com

CALIBRATION OF RADIOCARBON AGE TO CALENDAR YEARS

(Variables: C13/C12=-24.9:lab. mult=1)

Laboratory number: **Beta-163256**


Conventional radiocarbon age: **9390±40 BP**

2 Sigma calibrated result: **Cal BC 8750 to 8570 (Cal BP 10700 to 10520)**
(95% probability)

Intercept data

Intercept of radiocarbon age
with calibration curve: **Cal BC 8630 (Cal BP 10580)**

1 Sigma calibrated result: **Cal BC 8720 to 8610 (Cal BP 10670 to 10560)**
(68% probability)

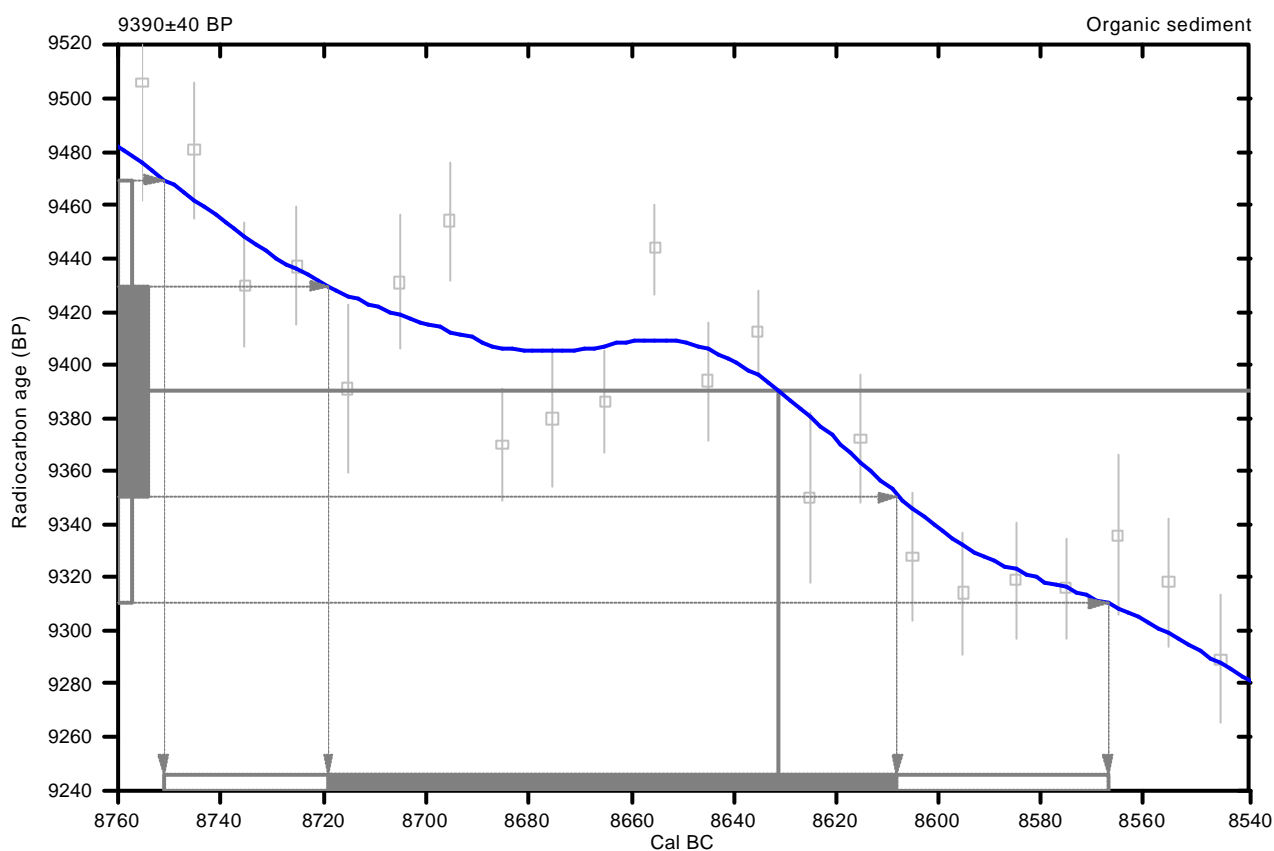

References:

Database used

Calibration Database
Editorial Comment

Stuiver, M., van der Plicht, H., 1998, *Radiocarbon* 40(3), pxii-xiii
INTCAL98 Radiocarbon Age Calibration

Stuiver, M., et. al., 1998, *Radiocarbon* 40(3), p1041-1083

Mathematics

A Simplified Approach to Calibrating C14 Dates

Talma, A. S., Vogel, J. C., 1993, *Radiocarbon* 35(2), p317-322

Beta Analytic Inc.

4985 SW 74 Court, Miami, Florida 33155 USA • Tel: (305) 667 5167 • Fax: (305) 663 0964 • E-Mail: beta@radiocarbon.com

CALIBRATION OF RADIOCARBON AGE TO CALENDAR YEARS

(Variables: C13/C12=-22.4:lab. mult=1)

Laboratory number: **Beta-163759**


Conventional radiocarbon age: **5290±70 BP**

2 Sigma calibrated result: **Cal BC 4320 to 3960 (Cal BP 6270 to 5920)**
(95% probability)

Intercept data

Intercept of radiocarbon age
with calibration curve: **Cal BC 4060 (Cal BP 6010)**

1 Sigma calibrated result: **Cal BC 4230 to 3990 (Cal BP 6180 to 5940)**
(68% probability)

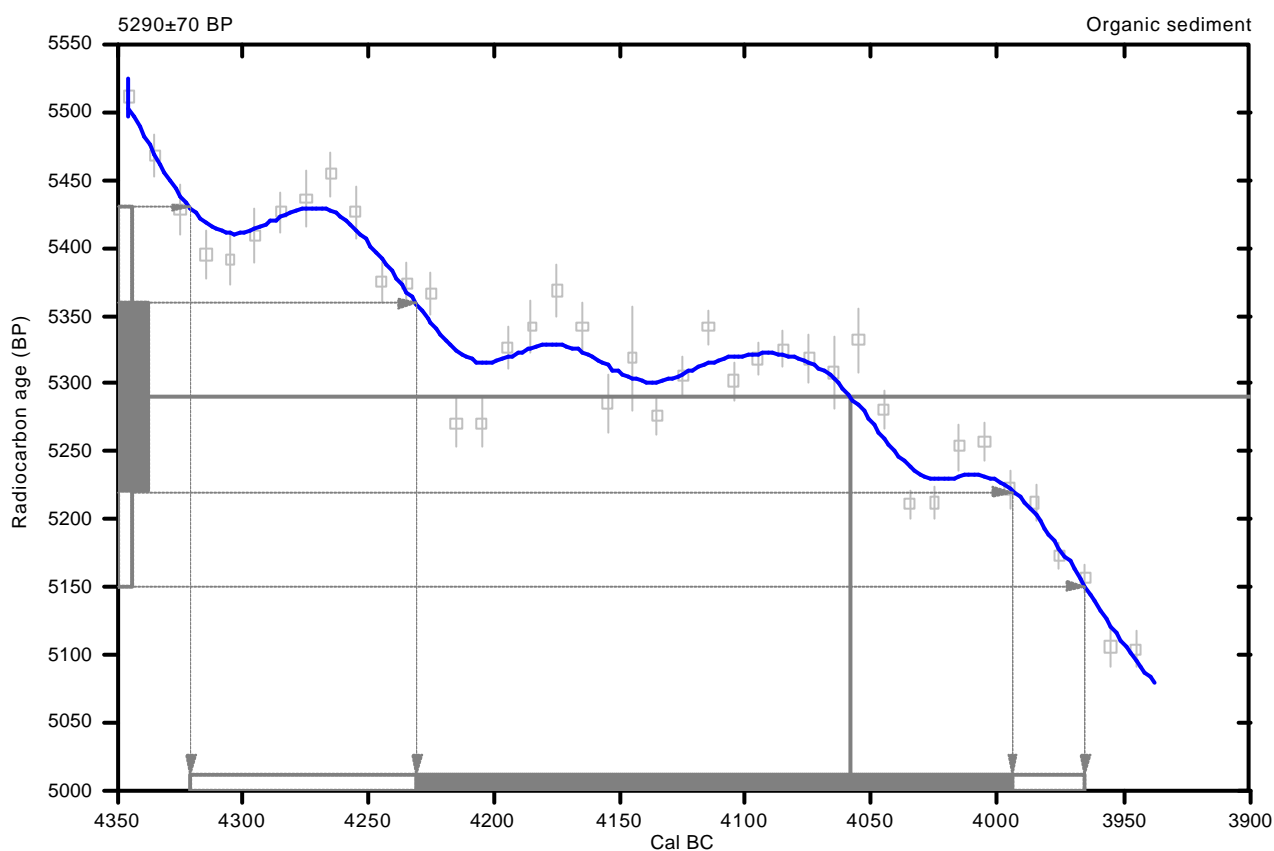

References:

Database used

Calibration Database
Editorial Comment

Stuiver, M., van der Plicht, H., 1998, Radiocarbon 40(3), pxii-xiii

INTCAL98 Radiocarbon Age Calibration

Stuiver, M., et. al., 1998, Radiocarbon 40(3), p1041-1083

Mathematics

A Simplified Approach to Calibrating C14 Dates

Talma, A. S., Vogel, J. C., 1993, Radiocarbon 35(2), p317-322

Beta Analytic Inc.

4985 SW 74 Court, Miami, Florida 33155 USA • Tel: (305) 667 5167 • Fax: (305) 663 0964 • E-Mail: beta@radiocarbon.com

CALIBRATION OF RADIOCARBON AGE TO CALENDAR YEARS

(Variables: C13/C12=-25.1:lab. mult=1)

Laboratory number: **Beta-163760**


Conventional radiocarbon age: **5590±80 BP**

2 Sigma calibrated result: **Cal BC 4580 to 4320 (Cal BP 6530 to 6270)**
(95% probability)

Intercept data

Intercept of radiocarbon age
with calibration curve: **Cal BC 4440 (Cal BP 6390)**

1 Sigma calibrated result: **Cal BC 4490 to 4350 (Cal BP 6440 to 6300)**
(68% probability)

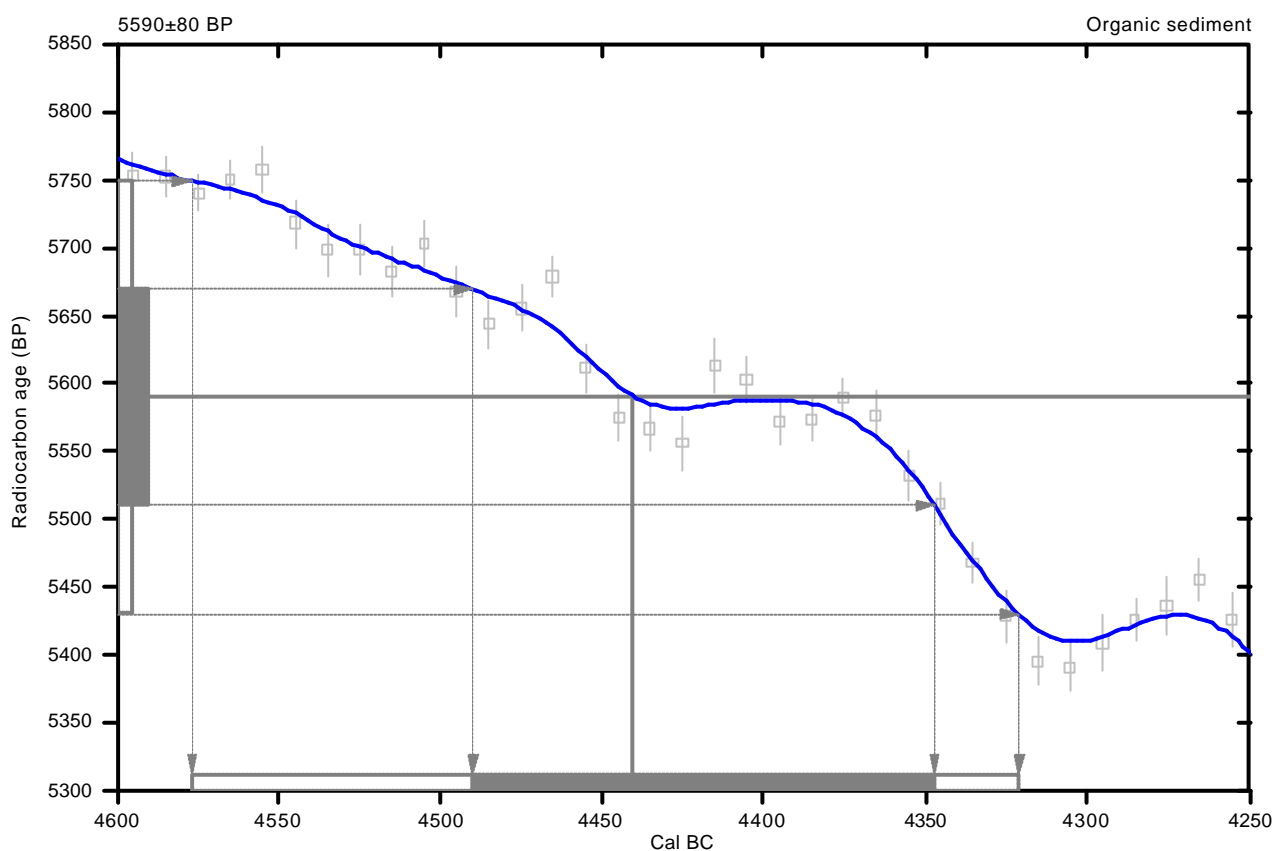

References:

Database used

Calibration Database
Editorial Comment

Stuiver, M., van der Plicht, H., 1998, Radiocarbon 40(3), pxii-xiii

INTCAL98 Radiocarbon Age Calibration

Stuiver, M., et. al., 1998, Radiocarbon 40(3), p1041-1083

Mathematics

A Simplified Approach to Calibrating C14 Dates

Talma, A. S., Vogel, J. C., 1993, Radiocarbon 35(2), p317-322

Beta Analytic Inc.

4985 SW 74 Court, Miami, Florida 33155 USA • Tel: (305) 667 5167 • Fax: (305) 663 0964 • E-Mail: beta@radiocarbon.com